



	Description
1 209063	MICS handpiece

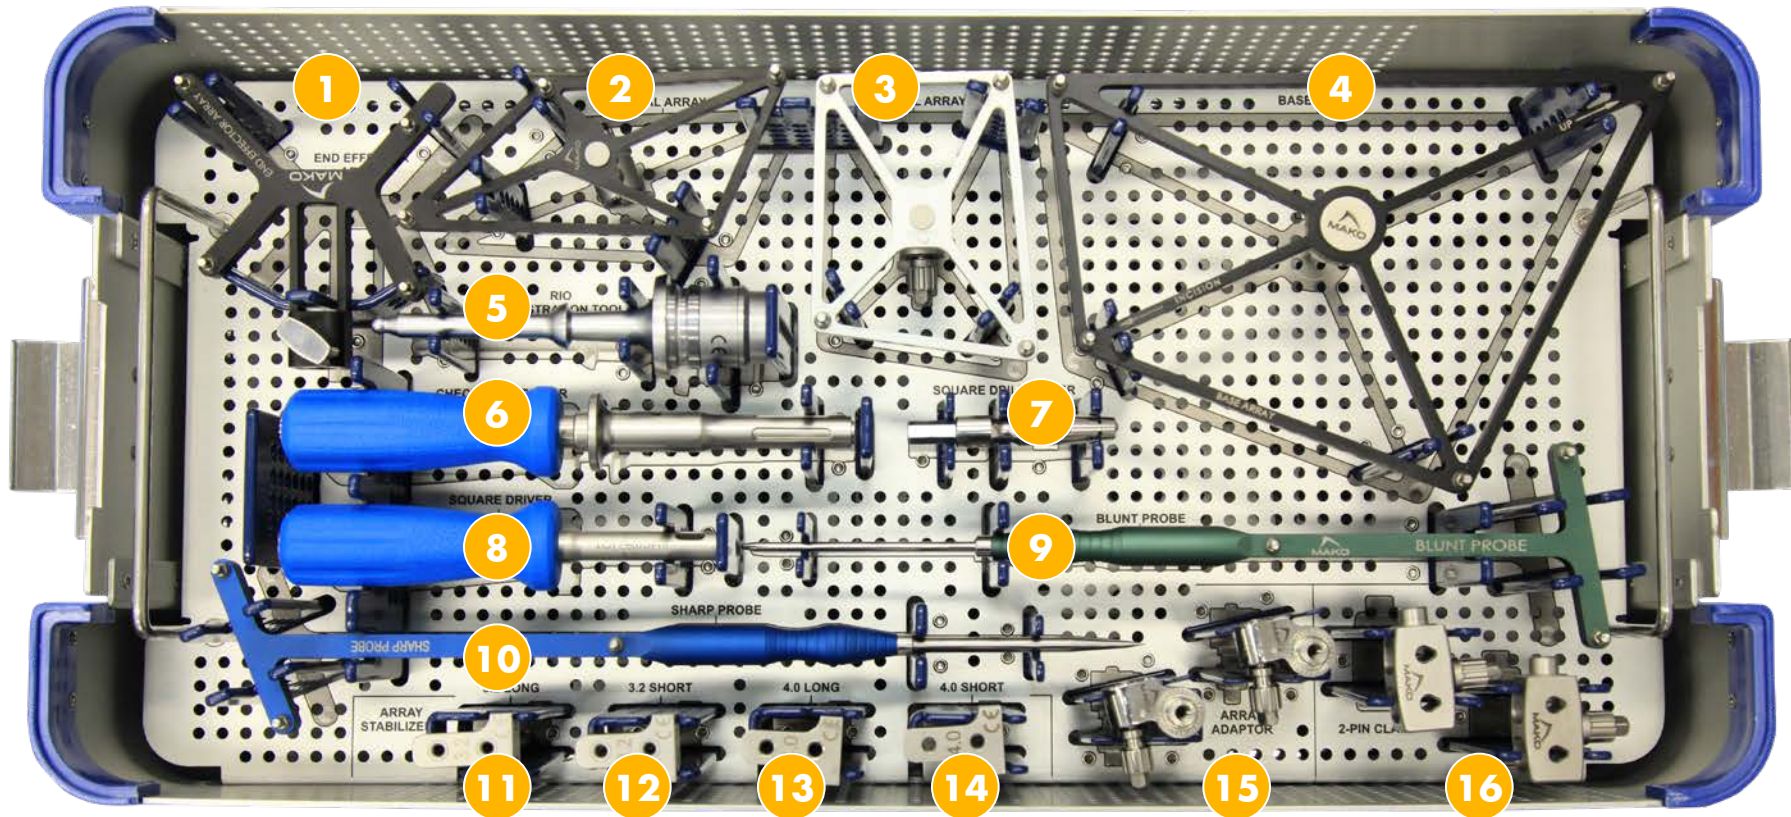

Upper tray #151202

	Description		Description		
1	110730	End effector array	9	110800	Blunt probe
2	112280	Tibial array	10	110810	Sharp probe
3	112290	Femoral array	11	112670	Long 3.2 array stabilizer*
4	112227	Base array	12	112690	Short 3.2 array stabilizer*
5	164020	Registration tool	13	112660	Long 4.0 array stabilizer*
6	110100	Knee checkpoint driver	14	112680	Short 4.0 array stabilizer*
7	111120	Square drill adaptor	15	112240	Array adaptor (2)
8	111160	Square driver	16	112270	2-Pin clamp (2)

*Optional instrument

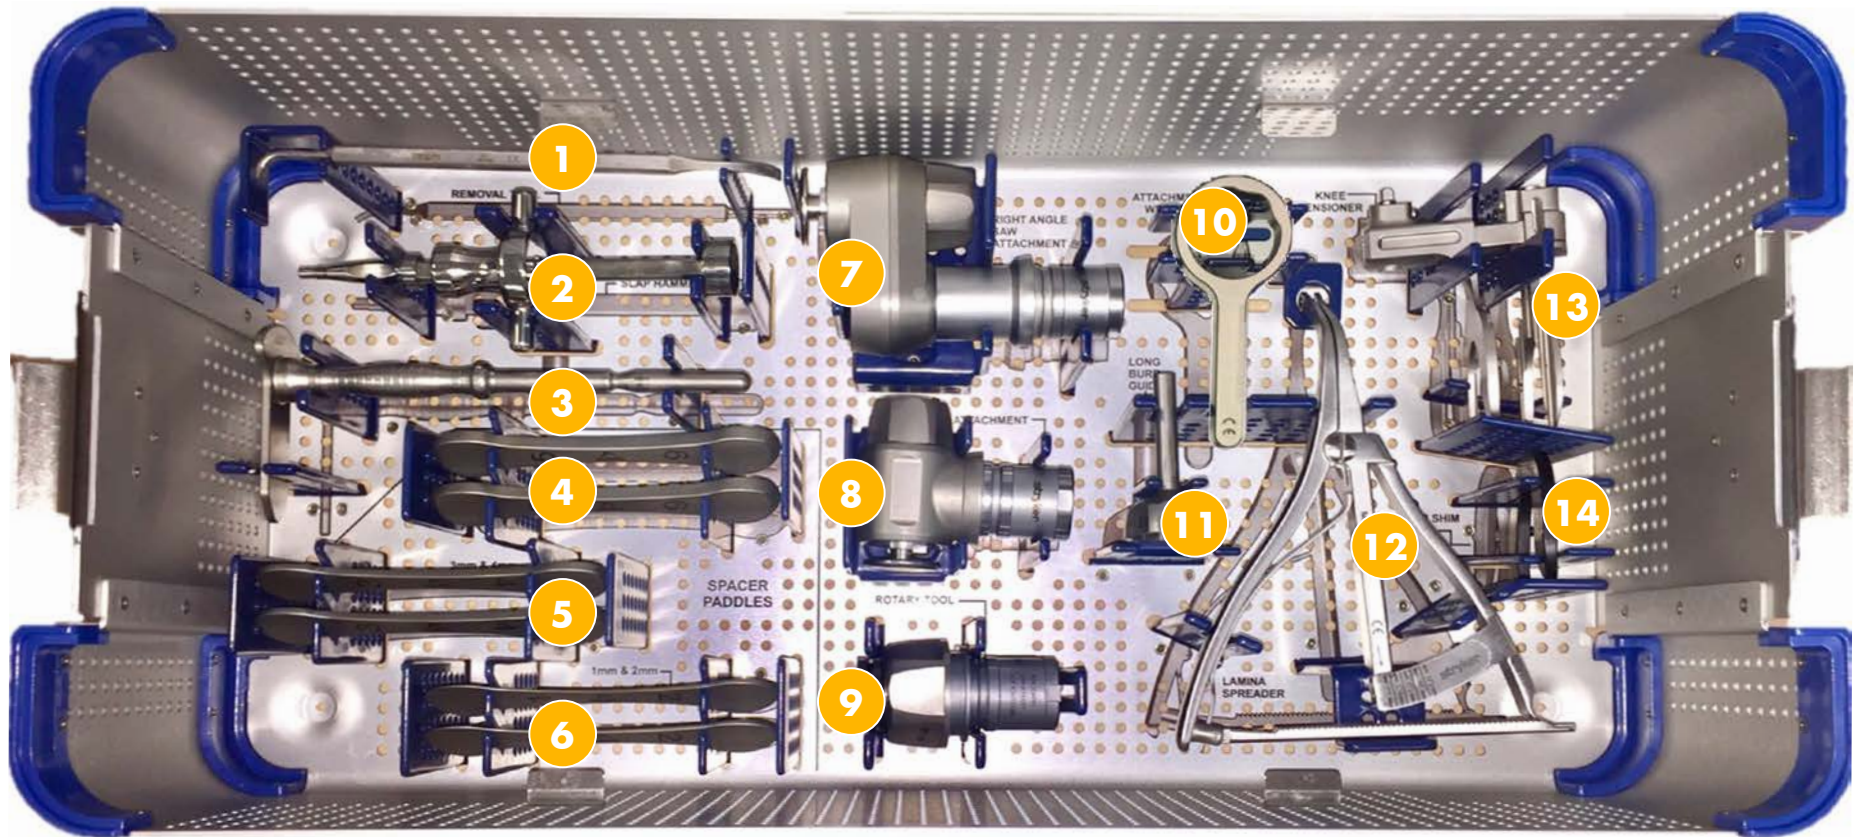

Lower tray #151201

		Description
1	120095	Cement removal tool
2	111140	Femoral trial slaphammer*
3	164100	Planar probe*
4	164505-03	Spacer paddle 5 × 6mm (2)
5	164505-02	Spacer paddle 3 × 4mm (2)
6	164505-01	Spacer paddle 1 × 2mm (2)
7	212480	Angled saw attachment*
8	212186	Straight saw attachment*

		Description
9	204990	Rotary attachment*
10	214015	Attachment wrench
11	204992	Long guard*
12	164306	Lamina spreader*
13	164206	Knee tensioner*
14	164006	Spacer shim, 5mm*

*Optional instrument




Upper tray

	Description
1	17060X Baseplate trials LM/RL ¹
2	17070X-X Insert onlay trials ²
3	17061X Baseplate trials RM/LL ³


	Description
4	17050X Femoral trials LM/RL
5	17051X Femoral trials RM/LL

1. Left column silver trays
 2. Multi-color disk rows
 3. Right column silver trays

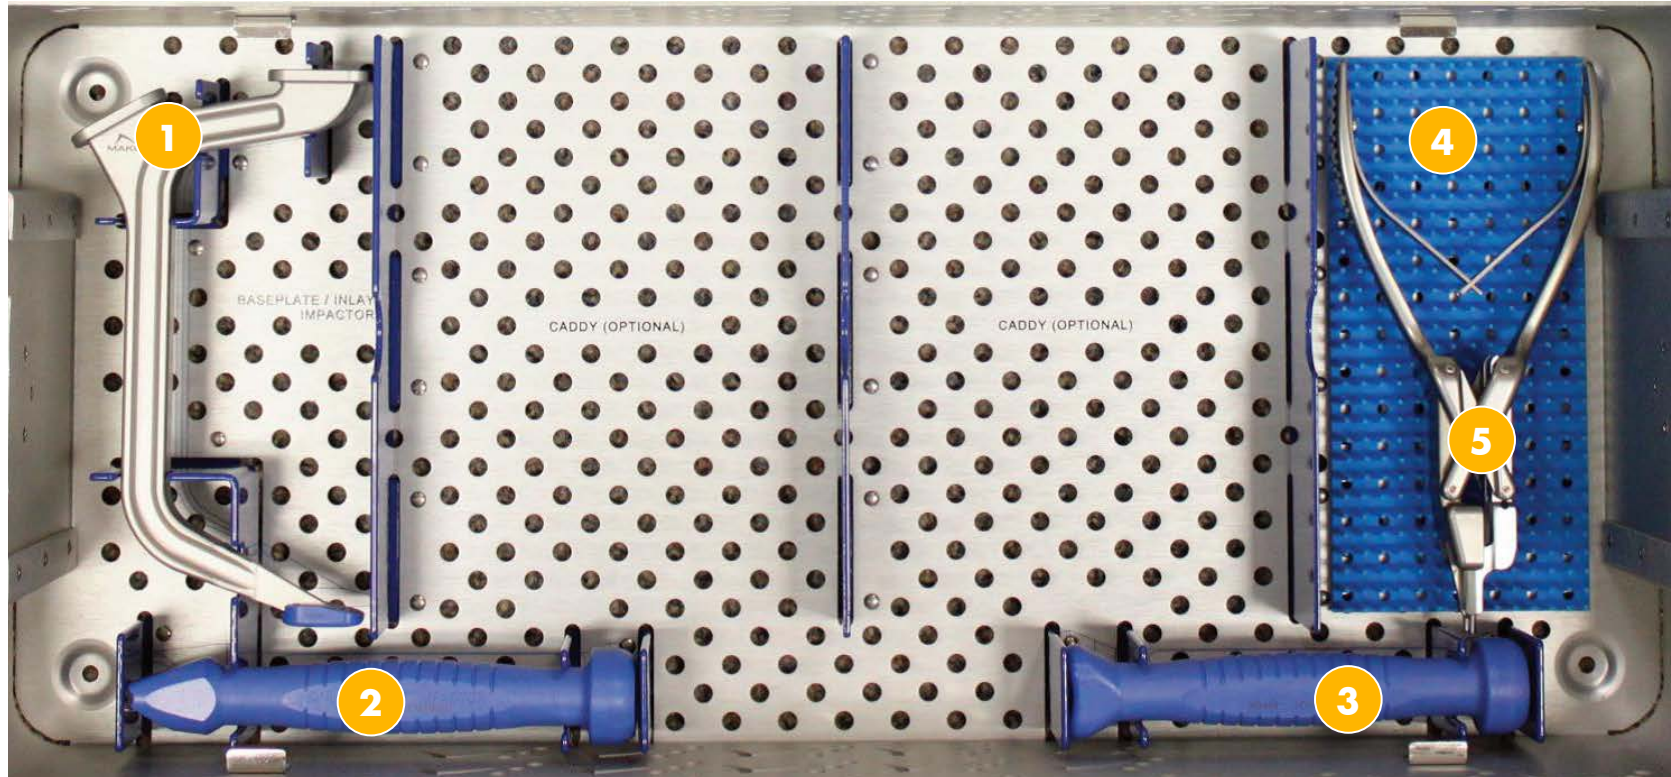

Lower tray


		Description
1	160195 (consists of 160173 and 160177)	Baseplate impactor
2	160405 (160185)	Onlay insert impactor
3	160402 (160175)	Femoral impactor
4	150068	Pin mat, blue w/ bumps, 3.5" x 7.5"*
5	160430	Onlay insert extractor*

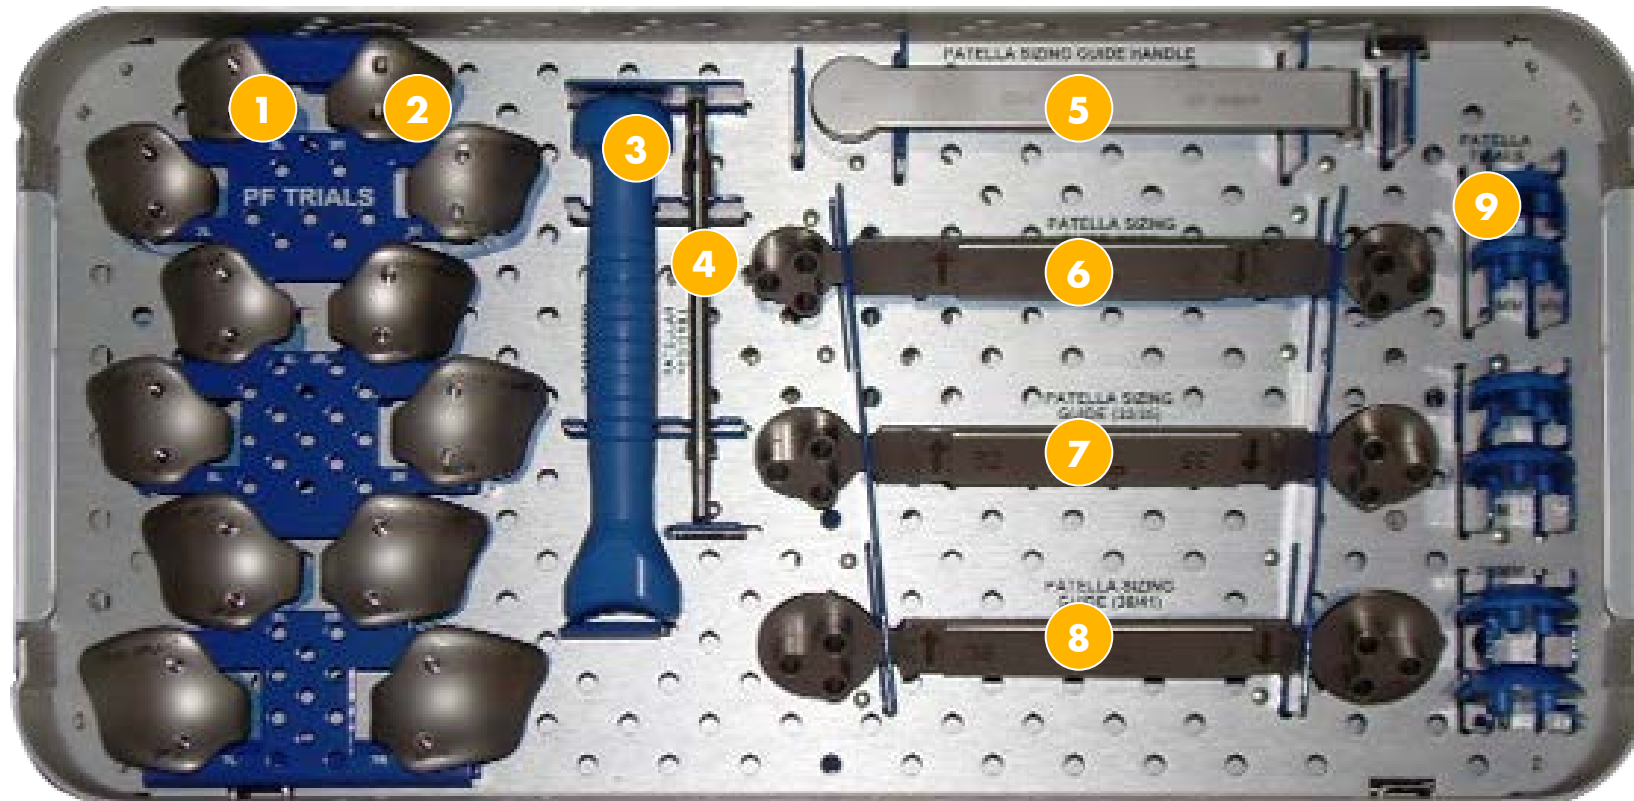

Upper tray


	Description
1	17040X Patellofemoral trials, left
2	17041X Patellofemoral trials, right
3	160403 (160180) Patellofemoral impactor
4	160171 Patellar/tibial peg drill
5	111540 Patella sizing guide handle

	Description
6	111541-1 Patella sizing guide (26mm/29mm)
7	111541-2 Patella sizing guide (32mm/35mm)
8	111541-3 Patella sizing guide (38mm/41mm)
9	170320-X Patella round dome trials

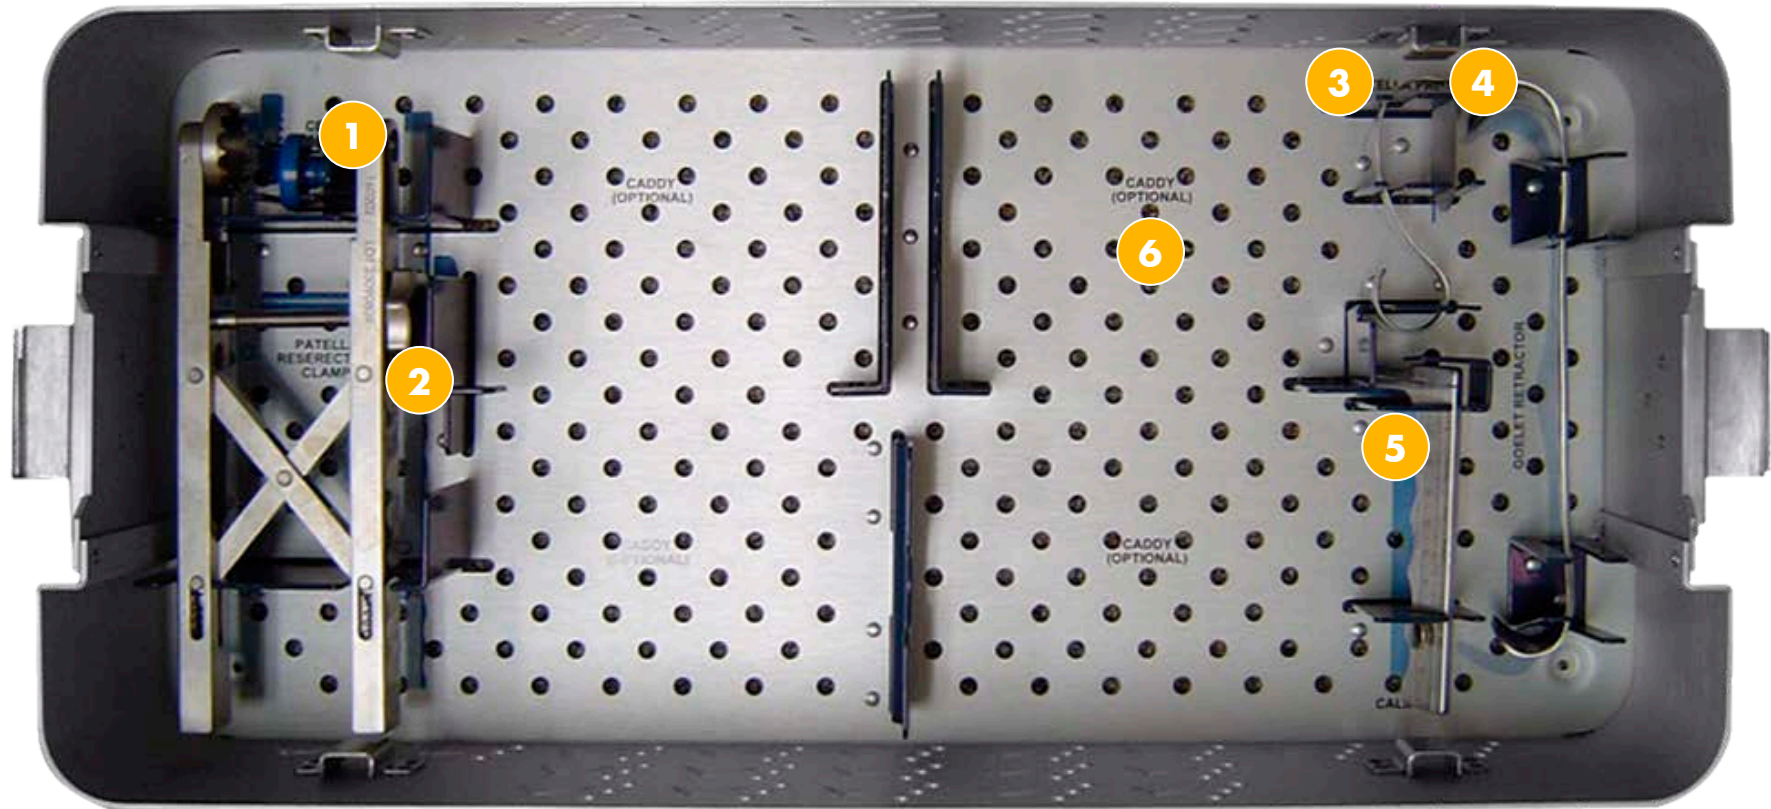

Lower tray

	Description		Description		
1	160205	Cement clamp body	4	160170	Goelet retractor
2	160202	Patella resection clamp	5	111560	Townley caliper
3	111550	Patella protector	6	150077	Patellofemoral saw guide caddy*

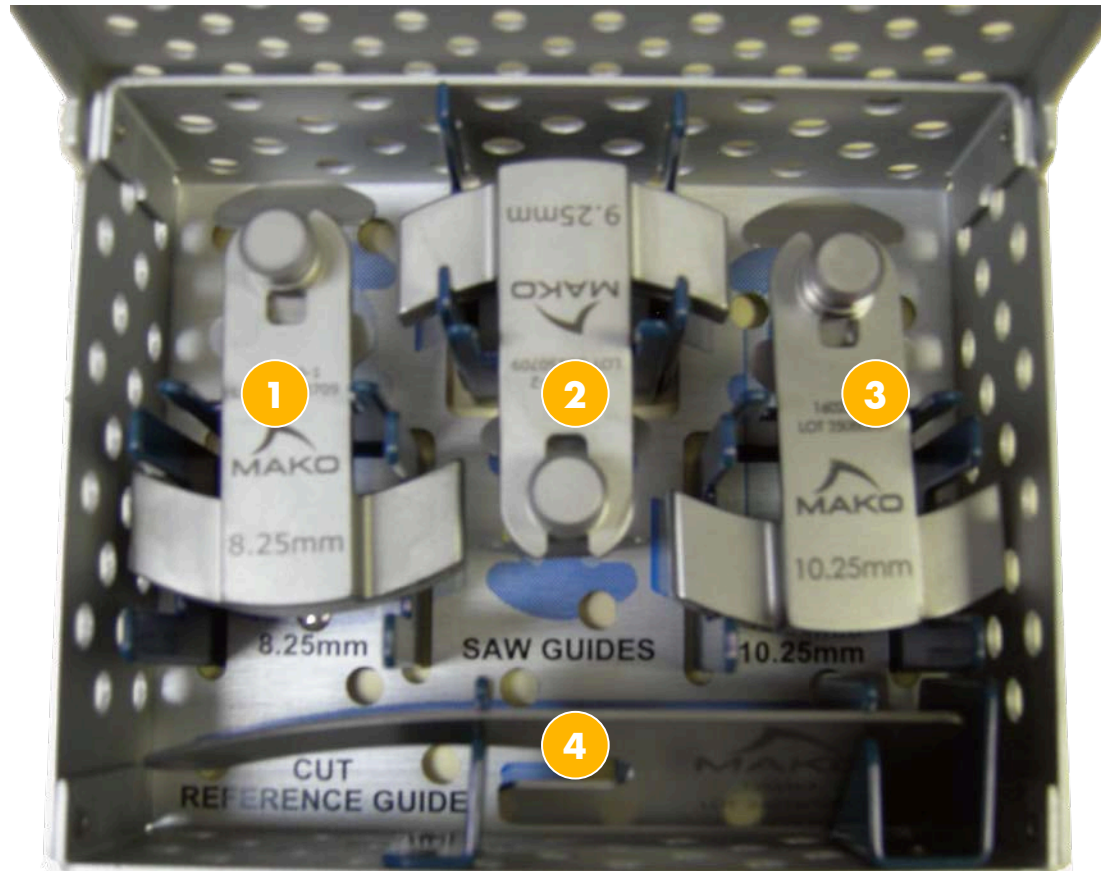

Optional caddy

	Description
1 160220-1	Saw guide, 8.25mm
2 160220-2	Saw guide, 9.25mm


	Description
3 160220-3	Saw guide, 10.25mm
4 120063	Anterior cut reference guide



Optional tray

	Description
1	170501 Femoral trial, size 1 LM/RL
2	170511 Femoral trial, size 1 RM/LL
3	170701-1 Insert onlay trial, size 1 × 8mm
4	170701-2 Insert onlay trial, size 1 × 9mm
5	170701-3 Insert onlay trial, size 1 × 10mm
6	170601 Baseplate trial, size 1 LM/RL

	Description
7	170611 Baseplate trial, size 1 RM/LL
8	160141 Femoral template, size 1 LM/RL
9	160151 Femoral template, size 1 RM/LL
10	160121 Baseplate template, size 1 LM/RL
11	160131 Baseplate template, size 1 RM/LL

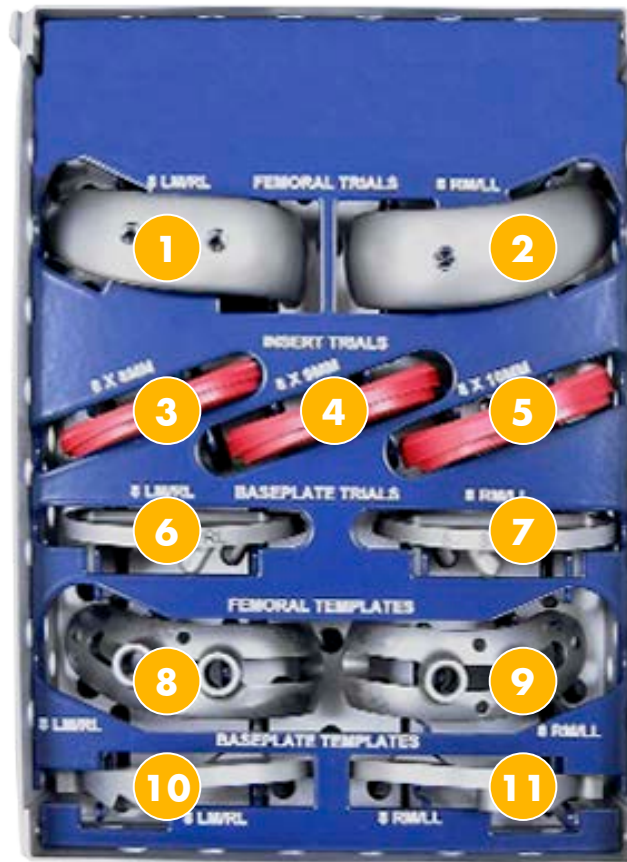

Optional tray

	Description
1	170508 Femoral trial, size 8 LM/RL
2	170518 Femoral trial, size 8 RM/LL
3	170708-1 Insert onlay trial, size 8 × 8mm
4	170708-2 Insert onlay trial, size 8 × 9mm
5	170708-3 Insert onlay trial, size 8 × 10mm
6	170608 Baseplate trial, size 8 LM/RL


	Description
7	170618 Baseplate trial, size 8 RM/LL
8	160148 Femoral template, size 8 LM/RL
9	160158 Femoral template, size 8 RM/LL
10	160128 Baseplate template, size 8 LM/RL
11	160138 Baseplate template, size 8 RM/LL



Optional tray

	Description
1	170701-5 Tibial insert onlay trial, size 1 × 12mm
2	170702-5 Tibial insert onlay trial, size 2 × 12mm
3	170703-5 Tibial insert onlay trial, size 3 × 12mm
4	170704-5 Tibial insert onlay trial, size 4 × 12mm

	Description
5	170705-5 Tibial insert onlay trial, size 5 × 12mm
6	170706-5 Tibial insert onlay trial, size 6 × 12mm
7	170707-5 Tibial insert onlay trial, size 7 × 12mm
8	170708-5 Tibial insert onlay trial, size 8 × 12mm

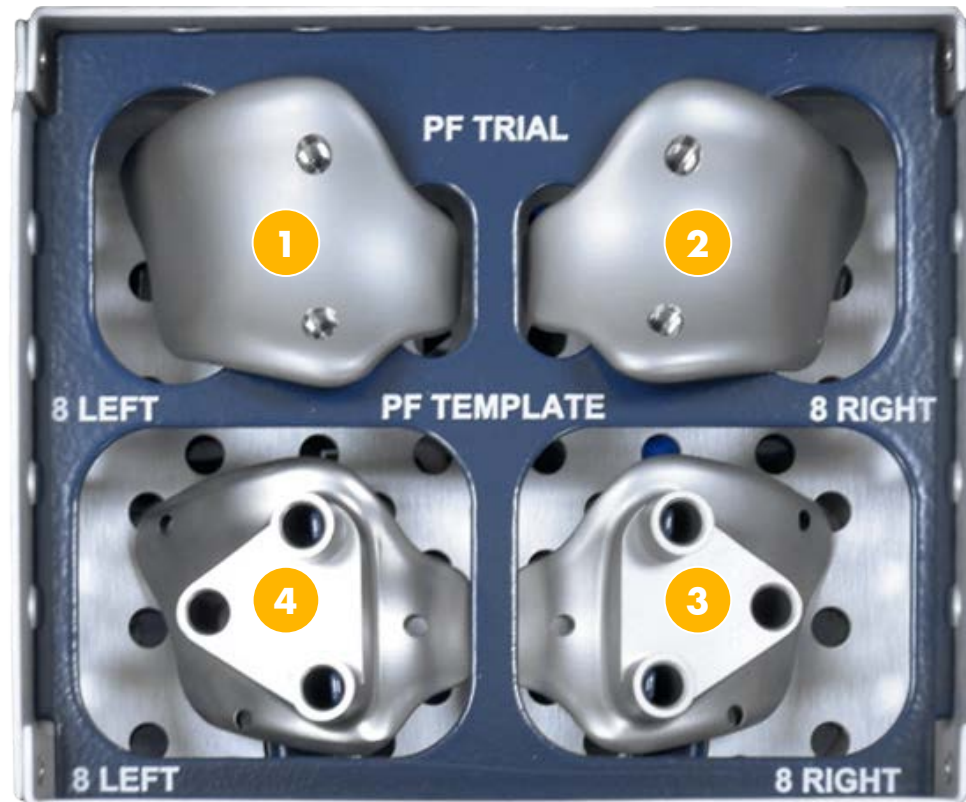

Optional tray

Description

- 1 170408 Patellofemoral trial, size 8 left
- 2 170418 Patellofemoral trial, size 8 right

Description

- 3 160118 Patellofemoral template, size 8 right
- 4 160108 Patellofemoral template, size 8 left

A surgeon must always rely on his or her own professional clinical judgment when deciding whether to use a particular product when treating a particular patient. Stryker does not dispense medical advice and recommends that surgeons be trained in the use of any particular product before using it in surgery.

The information presented is intended to demonstrate the breadth of Stryker's product offerings. A surgeon must always refer to the package insert, product label and/or instructions for use before using any Stryker product. The products depicted are CE marked according to the Medical Device Directive 93/42/EEC. Products may not be available in all markets because product availability is subject to the regulatory and/or medical practices in individual markets. Please contact your sales representative if you have questions about the availability of Stryker's products in your area.

Stryker Corporation or its divisions or other corporate affiliated entities own, use or have applied for the following trademarks or service marks: Mako, Stryker. All other trademarks are trademarks of their respective owners or holders.